

**SHENTEK**

# **Residual PG13 DNA Size Analysis Kit User Guide**

Version: A/0

For Research Use Only

Product No.: 1103178

Reagents for  $3 \times 100$  Reactions

**Huzhou Shenke Biotechnology Co., Ltd**

*(IMPORTANT: Please read this document carefully before experiment.)*

## 1. Product information

### ■ Product description

SHENTEK® Residual PG13 DNA Size Analysis Kit is used to quantitate PG13 host DNA residues of different fragment sizes in different stages of biopharmaceutical products, from in-process samples to final products.

This kit utilizes fluorescent quantitative PCR technique (FAM) to perform rapid and specific quantitation of residual PG13 DNA fragments in samples. The assay is designed to amplify three different fragments (118bp, 212bp, 502bp) for determining the accurate size distribution, and the limit of detection (LOD) reaches femtograms (fg) level. For extraction information, please refer to the SHENTEK® Residual Host Cell DNA Sample Preparation Kit User Guide (Product No. 1104191).

### ■ Kit contents and storage

*WARNING: Please read the Material Safety Data Sheets (MSDSs) and follow the handling instructions. Wear appropriate protective eyewear, mask, clothing, and gloves.*

Table 1. Kit components and storage

Reagent	Part No.	Quantity	Storage
PG13 DNA Control	NNA049	50 $\mu$ L $\times$ 1 tube	-20°C
qPCR Reaction Buffer	NNB001	850 $\mu$ L $\times$ 6 tubes	-20°C, protect from light
PG13 Primer&Probe MIX-118	NNC083	300 $\mu$ L $\times$ 1 tube	
PG13 Primer&Probe MIX-212	NNC084	300 $\mu$ L $\times$ 1 tube	
PG13 Primer&Probe MIX-502	NNC085	300 $\mu$ L $\times$ 1 tube	
IPC MIX	NNC070	550 $\mu$ L $\times$ 1 tube	
DNA Dilution Buffer (DDB)	NND001	1.5 mL $\times$ 3 tubes	-20°C

The kit components can be stored at appropriate conditions for up to 24 months.

Please check the expiration date on the labels.

## ■ Applied instruments, including but not limited to the following

- SHENTEK-96S Real-Time PCR System
- 7500 Real-Time PCR system
- Lightcycler 480 Real-Time PCR System


## ■ Required materials not included in the kit

- Nonstick, DNase-free & Low Retention Microfuge Tubes, 1.5 mL
- Nonstick, Low Retention Tips: 1000  $\mu$ L, 100  $\mu$ L and 10  $\mu$ L
- 96-well qPCR plates with sealing film or PCR 8-strip tubes with caps

## ■ Related equipments

- Real-Time PCR system
- Benchtop microcentrifuge
- Vortex mixer
- Micropipettes: 1000  $\mu$ L, 100  $\mu$ L and 10  $\mu$ L

## ■ Workflow

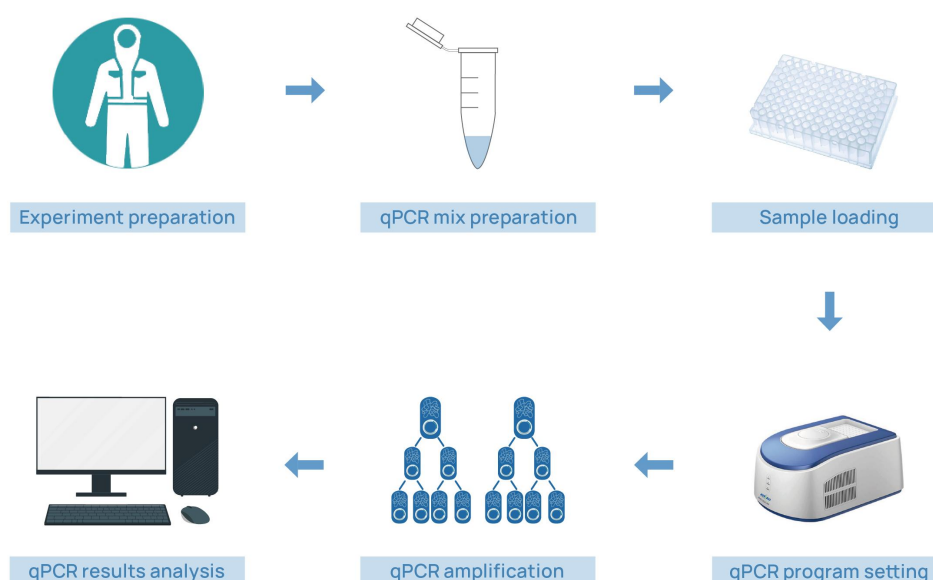

## 2. Methods

### ■ Experiment preparation

1. Wear appropriate protective eyewear, clothing, mask and gloves.
2. Irradiate the tabletop, pipettes and tubes with UV for 30 minutes, and disinfect with 75% ethanol.
3. Thaw the kit completely at 2-8 °C or melt on ice, vortex and spin briefly.

### ■ DNA Control serial dilutions for the standard curve

*Note: The kit contains three PG13 primer & probe sets for different fragment lengths. Please set up three separate standard curves corresponding to each fragment length.*

Please check the concentration labeled on the tube containing the PG13 DNA Control prior to dilution.

Prepare three sets of PG13 DNA Control solution with DNA Dilution Buffer (DDB) following the serial dilution procedure below:

1. Thaw PG13 DNA Control and DDB completely at 2-8°C or melt on ice. Vortex to mix well and quickly spin down the reagents for 3-5 seconds in microcentrifuge, and repeat 3 times.
2. Label six nonstick 1.5 mL centrifuge tubes: ST0, ST1, ST2, ST3, ST4 and ST5.
3. Dilute the DNA Control to 3000 pg/μL with DDB in the ST0 tube. Vortex to mix well and quickly spin down the reagents for 3-5 seconds in microcentrifuge, and repeat 3 times to mix thoroughly.
4. Add 180 μL DDB to each tube of ST1, ST2, ST3, ST4 and ST5.
5. Perform the serial dilutions according to Table 2:
  - a. Transfer 20 μL of the DNA control from tube ST0 to ST1, then vortex to mix well and quickly spin down the reagents for 3-5 seconds in microcentrifuge. Repeat vortex and spin for 3 times.
  - b. Continue to transfer 20 μL of DNA control solution from the previous dilution tube to the next until you reach tube ST5.

Table 2. Dilution for PG13 DNA Control

Serial dilution tube	Dilution	Conc. (pg/ $\mu$ L)
ST0	Dilute the DNA Control with DDB	3000
ST1	20 $\mu$ L ST0 + 180 $\mu$ L DDB	300
ST2	20 $\mu$ L ST1 + 180 $\mu$ L DDB	30
ST3	20 $\mu$ L ST2 + 180 $\mu$ L DDB	3
ST4	20 $\mu$ L ST3 + 180 $\mu$ L DDB	0.3
ST5	20 $\mu$ L ST4 + 180 $\mu$ L DDB	0.03

- *The remaining unused DDB need to be stored at 2-8°C. If the solution is cloudy or contains precipitates, heat at 37°C until it clear.*
- *At least five concentration of standard curve should be included. To select appropriate sample dilutions, we recommend to perform method validation before sample testing*

### ■ Negative Control Sample (NCS) preparation

Add 100  $\mu$ L of DDB to a new 1.5 mL microfuge tube, and label as NCS.

NCS and samples should be prepared in same way during DNA extraction.

### ■ qPCR MIX preparation

1. Determine the number of reaction wells based on your selected standard curve, with the number of test samples and control samples. Generally, triplicates are tested for each sample.

Number of reaction wells = (standard curve of 5 concentration gradients + 1 NTC + 1 NCS + test samples )  $\times$  3

2. Prepare qPCR MIX according to Table 3, 4 and 5.

Table 3. qPCR MIX-118 preparation

Reagents	Volume/reaction	Volume for 30 reaction (includes 10% overage)
qPCR Reaction Buffer	15.9 $\mu$ L	524.7 $\mu$ L
PG13 Primer&Probe MIX-118	2.8 $\mu$ L	92.4 $\mu$ L
IPC MIX	1.3 $\mu$ L	42.9 $\mu$ L
Total volume	20 $\mu$ L	660 $\mu$ L

Table 4. qPCR MIX-212 preparation

Reagents	Volume/reaction	Volume for 30 reaction (includes 10% overage)
qPCR Reaction Buffer	15.9 $\mu$ L	524.7 $\mu$ L
PG13 Primer&Probe MIX-212	2.8 $\mu$ L	92.4 $\mu$ L
IPC MIX	1.3 $\mu$ L	42.9 $\mu$ L
Total volume	20 $\mu$ L	660 $\mu$ L

Table 5. qPCR MIX-502 preparation

Reagents	Volume/reaction	Volume for 30 reaction (includes 10% overage)
qPCR Reaction Buffer	15.9 $\mu$ L	524.7 $\mu$ L
PG13 Primer&Probe MIX-502	2.8 $\mu$ L	92.4 $\mu$ L
IPC MIX	1.3 $\mu$ L	42.9 $\mu$ L
Total volume	20 $\mu$ L	660 $\mu$ L

*For simultaneous detection of the three fragments, please prepare at least 90  $\mu$ L template DNA for three assays.*

- Mix thoroughly and place on ice, aliquot 20  $\mu$ L/well into 96-well qPCR plate or PCR 8-strip tubes.

## ■ qPCR Reaction MIX preparation

- Prepare qPCR Reaction MIX following Table 6 - 8, and 96-well plate layout template is shown in Table 9.

Table 6. qPCR Reaction MIX-118 preparation

<b>Tubes</b>	<b>ST-118</b>	<b>NTC</b>	<b>NCS</b>	<b>Test sample</b>
qPCR MIX	20 µL	20 µL	20 µL	20 µL
Samples	10 µL ST1 - ST5	10 µL DDB	10 µL purified NCS	10 µL purified test sample
Total Volume	30 µL	30 µL	30 µL	30 µL

Table 7. qPCR Reaction MIX-212 preparation

<b>Tubes</b>	<b>ST-212</b>	<b>NTC</b>	<b>NCS</b>	<b>Test sample</b>
qPCR MIX	20 µL	20 µL	20 µL	20 µL
Samples	10 µL ST1 - ST5	10 µL DDB	10 µL purified NCS	10 µL purified test sample
Total Volume	30 µL	30 µL	30 µL	30 µL

Table 8. qPCR Reaction MIX-502 preparation

<b>Tubes</b>	<b>ST-502</b>	<b>NTC</b>	<b>NCS</b>	<b>Test sample</b>
qPCR MIX	20 µL	20 µL	20 µL	20 µL
Samples	10 µL ST1 - ST5	10 µL DDB	10 µL purified NCS	10 µL purified test sample
Total Volume	30 µL	30 µL	30 µL	30 µL

Table 9. Example of 96-well plate layout

Plate 1:

MIX-118						MIX-212						
NTC	NTC	NTC				NTC	NTC	NTC				A
NCS	NCS	NCS				NCS	NCS	NCS				B
												C
			ST5	ST5	ST5				ST5	ST5	ST5	D
S1	S1	S1	ST4	ST4	ST4	S1	S1	S1	ST4	ST4	ST4	E
S2	S2	S2	ST3	ST3	ST3	S2	S2	S2	ST3	ST3	ST3	F
S3	S3	S3	ST2	ST2	ST2	S3	S3	S3	ST2	ST2	ST2	G
S4	S4	S4	ST1	ST1	ST1	S4	S4	S4	ST1	ST1	ST1	H
1	2	3	4	5	6	7	8	9	10	11	12	

Plate 2:

MIX - 502												
NTC	NTC	NTC										A
NCS	NCS	NCS										B
												C
			ST5	ST5	ST5							D
S1	S1	S1	ST4	ST4	ST4							E
S2	S2	S2	ST3	ST3	ST3							F
S3	S3	S3	ST2	ST2	ST2							G
S4	S4	S4	ST1	ST1	ST1							H
1	2	3	4	5	6	7	8	9	10	11	12	

- *This example represents three assays, including selected standard curve points of PG13 DNA Control (ST1-ST5), 1 NTC, 1 NCS, and 4 test sample (S1-S4), with 3 replicates for each sample.*
- *The plate layout for sample loading can be adjusted based on the sample quantity.*

2. Seal the 96-well plate with sealing film. Mix well in microplate shaker, then spin down the reagents for 10 seconds in microcentrifuge and place it on the qPCR instrument.

## ■ qPCR program setting

*NOTE: The following instructions apply only to the ABI7500 instrument with SDS v1.4. If you use a different instrument or software, refer to the applicable instrument or software documentation.*

1. Create a new document, then in the Assay drop-down list, select **Standard Curve (Absolute Quantitation)**.
2. Click **New Detector**, then enter PG13-118 in the Name field, select **FAM** in the Reporter Dye drop-down list and select **(none)** in the Quencher Dye drop-down list, then click **OK**.
3. Create new detector for PG13-212 and PG13-502, separately as step2.
4. Click **New Detector**, then enter IPC in the Name field. Select **VIC** in the



Reporter Dye drop-down list and select **(none)** in the Quencher Dye drop-down list, then click **OK**.

5. Select **ROX** as the passive reference dye, then Click **Next**.
6. Select the applicable set of wells for the samples, then select the corresponding detector for each well.
7. Select Finish, and then set thermal-cycling conditions:
  - a. Set the thermal cycling reaction volume to 30 µL.
  - b. Set the temperature and time as follow in Table 10:

Table 10. qPCR running temperature and time

Step	Temp.	Time(mm:sec)	Cycles
Activation	95°C	10:00	1
Denaturation	95°C	00:15	40
Annealing	60°C	00:30	
Extension	72°C*	01:30	

\*Instrument will read the fluorescence signal during this step.


8. Save the document, then click **Start** to start the qPCR run.

## ■ Results analysis

1. Select **Set up** tab, then set tasks for each sample type by clicking on the Task Column drop-down list:
  - a. NTC: target DNA detector task = **NTC**
  - b. NCS, test samples= **Unknown**
2. Set up the standard curve as shown in the following table 11:

Table 11. Settings for Standard curve

Tube label	Task	Quantity (pg/µL)
ST1	Standard	300
ST2	Standard	30
ST3	Standard	3
ST4	Standard	0.3
ST5	Standard	0.03

3. Select the **Results** tab, then select Amplification Plot.
4. In the Data drop-down list, select **Delta Rn vs Cycle**.
5. In the Analysis Settings window, enter the following settings :
  - a. Select **Manual Ct**.
  - b. In the FAM Threshold field, enter 0.1. VIC Threshold field, enter 0.1.
  - c. Select **Automatic Baseline**.
6. Click the button  in the toolbar, then wait the plate analyzing.
7. Select the **Result** tab> >**Standard curve** tab, then verify the Slope, Intercept, R<sup>2</sup> values and Efficiency (Eff%).
8. Select the Report tab, then achieve the mean quantity and standard deviation for each sample.
9. Select **File > > Export > > Results**. In the Save as type drop-down list, select **Results Export Files**, then click **Save**.
10. For test samples, set the value of DNA size-118 to be 100%, calculate the percentage of the DNA size-212 and -502.
11. To analyze the Ct value of IPC, normally the mean Ct-IPC value of the sample should be within  $\pm 1.0$  of the NCS Ct-IPC value. If the mean Ct-IPC value of the sample is significantly higher than the Ct-IPC value of the NCS, this indicates that the sample may be inhibitory to the assay. We recommend to test the ERC samples in the same assay, and consider the sample recovery rate as priority.
12. The recovery rate of ERC samples is calculated based on the value of test samples and the ERC samples. The recovery rates should be between 50% and 150%.
13. The Ct value of NCS should be larger than the mean Ct value of the lowest concentration in the standard curve, and shows normal amplification curve in VIC signal channel. If the validated limit of quantitation (LOQ) concentration is less than the lowest concentration in the standard curve, the value of the NCS should be less than the concentration of LOQ.
14. The Ct value of NTC should be no less than 35.00 cycles or undetermined,

meanwhile shows normal amplification curve in VIC signal channel.

*Note: The parameter settings of the result analysis should be based on the specific model and the software version, and generally can also be automatically interpreted by the instrument.*

Effective date: 17 May 2024

## Support & Contact

The logo for SHENTEK, with the word in a bold, sans-serif font. The 'S' and 'H' are blue, and the 'E', 'N', 'T', 'E', 'K' are green.

Huzhou Shenke Biotechnology Co., Ltd.

[www.shentekbio.com](http://www.shentekbio.com)

Address: 8th Floor, 6B Building, No.1366 Hongfeng Road, Huzhou313000, Zhejiang Province, China

E-mail: [info@shentekbio.com](mailto:info@shentekbio.com)

Phone: +1 (908) 822-3199 / (+86) 400-878-2189